

Device Maintenance

Battery Replacement

Materials:
Replacement Battery (SR1154W)

- Remove the data logger from the egg enclosure
- Unscrew the knurled endcap on the data logger
- Tip the batteries (enclosed in a plastic sleeve) out of the enclosure tube.
- Use a small, dull, non-metallic tool (e.g. pen cap) to push the batteries out of the sleeve.
- Press the new batteries into the sleeve negative (-) end first.
- Place the sleeved batteries in the enclosure tube positive (+) end first.
- Screw the knurled cap back in place.

Battery Warning

WARNING: FIRE, EXPLOSION, AND SEVERE BURN HAZARD. DO NOT SHORT CIRCUIT, CHARGE, FORCE OVER DISCHARGE, DISASSEMBLE, CRUSH, PENETRATE OR INCINERATE. BATTERY MAY LEAK OR EXPLODE IF HEATED ABOVE 50°C (122°F).

Recalibration

The EggTemp-RH standard calibration is one point at 25°C and two points at 25%RH and 75%RH.

Pricing:

Recalibration traceable to NIST \$90.00
Recalibration \$70.00

Additional:


As Found Data \$15.00 per parameter/channel
Verification Point \$15.00 per point

To send the devices back, visit www.madgetech.com, select Services then RMA Process.

Part Number	EggTemp-RH
Temperature Sensor	Internal semiconductor
Temperature Range	0 to +60°C
Temperature Resolution	0.1°C
Temperature Accuracy	±0.5°C
Humidity Sensor	Internal semiconductor
Humidity Range	0 to 95%RH
Humidity Resolution	0.5% RH
Humidity Accuracy	±3.0%RH
Memory	16,383/channel
Sample Rate	2 seconds up to 12 hours
RH Units	%RH, dew pt., water vapor concentration (mg/ml)
Required Interface Package	IFC102 or IFC202
Baud Rate	38,400
Typical Battery Life	1 year
Operating Environment	0 to +60°C , 0 to 95%RH (non-condensing)
Submersible	No
Material	Enclosure: HDPE Logger: Stainless Steel
Dimensions	2.25" x 1.68" dia. (57.15mm x 42.67mm)
Approvals	-

Specifications subject to change.
See MadgeTech's terms and conditions at www.madgetech.com

EggTemp-RH

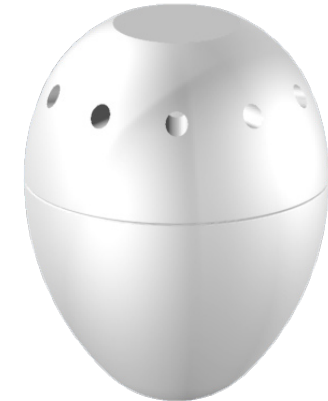

EggTemp-RH

Egg Temperature and Humidity Recorder

Authorized Distributor

Optimum Energy Products Ltd.

Website: www.dataloggerstore.com
Email: info@dataloggerstore.com
Toll free: 1.877.766.5412

Product Notes

LEDs

Once started, the LED will flash at the selected reading rate to indicate that the device is running. The LED will flash in one second intervals if there is an alarm condition.

Alarm Settings

To change the settings for the temperature alarm;

- Select **Alarm Settings** from the **Device menu** in the MadgeTech software. A window will appear allowing the customer to set the high and low temperature alarms.
- Press **Change** to edit the values.
- Check **Enable Alarm Settings** to enable the feature. The values can be entered in the field manually or by using the scroll bars.
- Click **Save** to save the changes. To clean an active alarm, press **Clear Alarm**.

Authorized Distributor

Optimum Energy Products Ltd.

Website: www.dataloggerstore.com
 Email: info@dataloggerstore.com
 Toll free: 1.877.766.5412

Installation Guide

Installing the Interface cable

- IFC200, IFC202 or IFC300
Refer to the "Quick Start Guide" included in the package.
- IFC110, IFC102 or IFC103
Plug the serial cable into the port and verify it is secure.
- USB-1 or USB-101
Install the USB drivers from the CD provided in the kit, than plug the USB cable into the computer and the serial cable into the serial port.

Installing the software

Insert the Software CD in the CD-ROM Drive. If the autorun does not appear, locate the drive on the computer and double click on **Autorun.exe**. Follow the instructions provided in the Wizard.

Connecting the data logger

- Once the software is installed and running, plug the interface cable into the data logger.
- Click the **Communication Menu**, then **Auto Configure Port**.
- After a moment, a box similar to the following will appear;




- Click **OK**. The **Device Status** box will appear. Click **OK**.
- At this point, communications have been configured for your logger. These settings can be found under the **Communication Menu**.

Note: For additional installation instructions refer to your "Data Logger & Software Operating Manual".

Device Operation

Starting the data logger

- Click **Device Menu** then **Start Device**.
- Choose the desired start method.
- Choose the start parameters by selecting a **Reading Rate** suitable for your application.
- Enter in any other desired parameters and click **Start**.
- A box will appear stating the data logger has been started. Click **OK**.

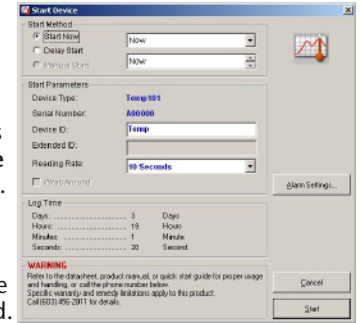

- Disconnect the data logger from the interface cable and place it in the environment to measure.

Note: The device will stop recording data when the end of memory is reached or the device is stopped. At this point the device cannot be restarted until it has been re-armed by the computer.

Downloading data from a data logger

- Connect the data logger to the interface cable.
- Click the **Device Menu** then **Read Device Data**. This will offload all recorded data onto the PC.

Technical Support

Visit www.madgetech.com, or call (603) 456-2011. Technical support is also available by e-mailing support@madgetech.com

Additional product information is available by e-mailing info@madgetech.com.